Disposable Suction and Irrigation Sets Instruction for use

【Product name】


Disposable Suction and Irrigation Sets

【Intended use】

The product is used for suction and irrigation of tissue or fluid in surgery.

【Structure】

Disposable Suction and Irrigation Sets is composed of Catheter, Negative pressure connector, Sucking and irrigating integrated tube, Robert clip, needle, needle cap, Sucking and irrigating valve, Rear cover Integrated tube mount, T-junction and Protective Cover. The structure is shown Fig.1 below:

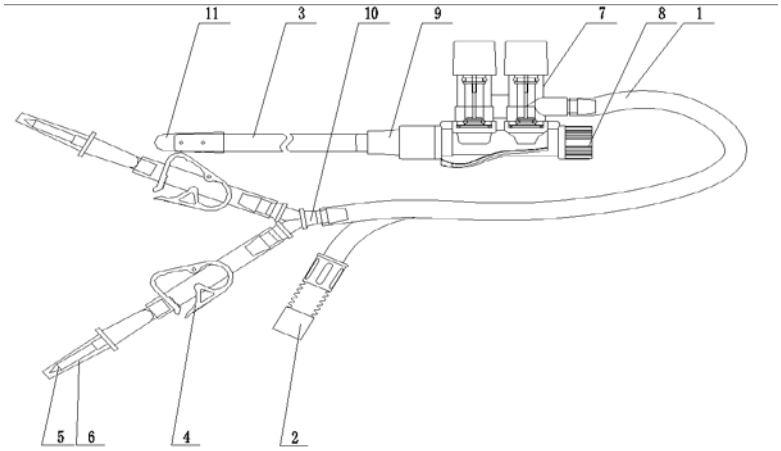

1- Catheter 2- Negative pressure connector 3- Sucking and irrigating integrated tube 4- Robert clip 5- needle 6- needle cap 7- Sucking and irrigating valve 8- Rear cover 9- Integrated tube mount 10- T-junction 11- Protective Cover

Fig. 1 Disposable Suction and Irrigation Sets

【Specifications】

WPSI5-330、WPSI5-420、WPSI10-330、WPSI10-420

【Main material】

Sucking and irrigating integrated tube（06Cr19Ni10）, Sucking and irrigating valve（PC）, needle, Robert clip, Rear cover and Integrated tube mount (ABS), Catheter, Negative pressure connector (PVC), T-junction(PP)

【Step of use】

1. Check the outer packaging to confirm no damage; Open the package and take out the product.

2. First, insert the needle into the saline bag, and then connect the negative pressure suction connector to the negative pressure suction device.

3. Open the Robert clip, until the whole connecting tube is filled with saline, adjust the negative pressure to 0.06MPa (450mmHg) or according to the professional doctor's requirements.

4. Finally, press and hold the sucking and irrigating valve to perform the suction and irrigation operations.

【Contraindication】


Patients who are not anesthetized are not allowed.

【Cautions】

1. The product has been sterilized with ethylene oxide, please don't use it if the package is damaged.
2. The product shall be used for one time, shall not be reused, and forbidden to be reused after reserialization;
3. The products are provided to professional doctors with certain basis knowledge and doctors after professional technical training.
4. Please read this instruction for uses carefully before using the product. Please destroy the product after use.
5. When using this product, the sterile operation specification shall be strictly implemented and the product is only for single use, destruction after use.
6. Do not use if the package is broken or expired before use.
7. Please check the wafer indicator on the sterilization package of this product. "red" means that this product is not sterilized by ethylene oxide and cannot be directly used.
8. "Green" indicates that the product has been sterilized with ethylene oxide and is ready for clinical use.
9. To avoid adverse consequences, please read the instructions carefully before use.
10. Please check whether the product is in the valid period before use. The sterilization period is three years. The product beyond the valid period is strictly prohibited to be used and sterilized again.

【Explanation of marks, sighs and abbreviations】

 KEEP DRY	 FRAGILE,HANDLE WITH CARE	 UPWARDS	 CAUTION

 USE-BY DATE	 MANUFACTURER	 DATE OF MANUFACTURE	 BATCH CODE
 DO NOT RE-USE	 DO NOT USE IF PACKAGE IS DAMAGED	 STERILIZED USING ETHYLENE OXIDE	 STERILE

【Storage】

The product should be stored in a dry room with excellent ventilation and without caustic gases.

The relative humidity of the room must be less than 80%.

【Transportation】

During transport, the product should avoid squeezing and rain. Handel with care and do not invert.

【Sterilization method】Ethylene oxide sterilization is used for the product.

【Sterilization period of validity】The sterilization period of validity is 3 years.

【Manufacturer】

Changzhou Weipu Medical Devices Co., Ltd

Add: NO.1-5, Chuangxin Avenue, Xinbei District, Changzhou, Jiangsu,China

Tel: 0519-69882737

【Authorized Representative】

Shanghai International Holding Corp. GmbH (Europe)

Add: Eiffestrasse 80, 20537 Hamburg，Germany

Tel: +49-40-2513175 Fax: +49-40-255726

Dimdi No. : DE/0000040627 E-mail: shholding@hotmail.com

CE 2292