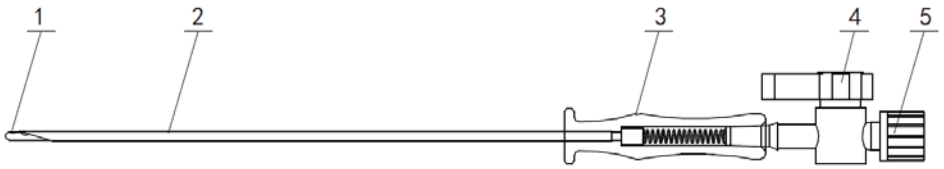
Disposable sterile pneumoperitoneum needle
Instruction for Use

【Product Name】Disposable sterile pneumoperitoneum needle

【Model No.】WPQF-120、WPQF-150

【Structure】

Disposable sterile pneumoperitoneum needle (hereinafter referred to as "pneumoperitoneum needle") consists of a puncture needle, a ventilation core, a handle, a cap and a two-way valve.



1. Ventilation core 2. Puncture needle 3. Handle 4. Two-way valve 5. Cap

Figure 1 Schematic diagram of the structure of pneumoperitoneum needle

【main Material】

Handle (PC), puncture needle (06Cr19Ni10)

【Application】

Used to establish pneumoperitoneum during abdominal endoscopic surgery.

【Population】

All persons

【Steps of use】

1. After checking that the product package is not damaged, open the product package and take out the pneumoperitoneum needle;

2. Aim the needle of the pneumoperitoneum needle at the site to be penetrated, and perform abdominal wall puncture with uniform force;

3. Then inject carbon dioxide gas into the abdominal cavity from the pneumoperitoneum needle to establish pneumoperitoneum;

4. After the pneumoperitoneum is completed and the requirements are met, pull out the pneumoperitoneum needle.

【Contraindication】

Those unable to perform anesthesia and laparoscopic surgery.

【Cautions】

1. The product has been sterilized with ethylene oxide. Please do not use it if the package is damaged.

2.The product shall be used for one time, shall not be reused, and forbidden to be reused after reserialization.

3.The products are provided to professional doctors with certain basis knowledge and doctors after professional technical training.

4.Please read this instruction for uses carefully before using the product. Please destroy the product after

use.

5.When using this product, the sterile operation specification shall be strictly implemented and the product is only for one-time use, destruction after use.

6. Do not use if the package is broken or expired before use.



7. Please check the wafer indicator on the sterilization package of this product. "red" means that this product is not sterilized by ethylene oxide and cannot be directly used.

"Green" indicates that the product has been sterilized with ethylene oxide and is ready for clinical use.

8. To avoid adverse consequences, please read the instructions carefully before use.

9. Please check whether the product is in the valid period before use. The sterilization period is three years. The product beyond the valid period is strictly prohibited to be used and sterilized again.

【Explanation of marks, sighs and abbreviations】

 KEEP DRY	 FRAGILE, HANDLE WITH CARE	 UPWARDS	 CAUTION
 USE-BY DATE	 MANUFACTURER	 DATE OF MANUFACTURE	 BATCH CODE
 DO NOT RE-USE	 DO NOT USE IF PACKAGE IS DAMAGED	 STERILIZED USING ETHYLENE OXIDE	 STERILE

【Storage】

The product should be stored in a dry room with excellent ventilation and without caustic gases. The relative humidity of the room must be less than 80%.

【Transportation】

During transport, the product should avoid squeezing and rain. Handel with care and do not invert.

【Sterilization method】 Ethylene oxide sterilization is used for the product.

【Sterilization period of validity】 The sterilization period of validity is 3 years.

【Manufacturer】

Changzhou Weipu Medical Devices Co., Ltd

Add: NO.1-5, Chuangxin Avenue, Xinbei District, Changzhou, Jiangsu,China Tel:

0519-69882737

【Authorized Representative】 EC REP

Shanghai International Holding Corp. GmbH (Europe) Add:

Eiffestrasse 80, 20537 Hamburg，Germany

Tel: +49-40-2513175 Fax: +49-40-255726

Dimdi No. : DE/0000040627 E-mail: shholding@hotmail.com